


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAR 11 2010

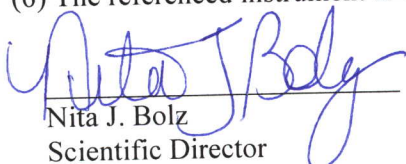
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130286 ✓
Name		Stan Swetof (Det.)	ID# 5002 Date 3/8/10 ✓
A	Agency	North Pole Police Dept.	Phone # 907-488-6902 ✓
Instrument Location		125 Snowman Lane, North Pole 99705 ✓	
B	Alco S/N	X172959 ✓	Target Value .083 ✓
	Alco Test Values		High Pressure 4500 PSI ✓
	1 st Alco .073 ✓		2 nd Alco .075 ✓
Signature		 ✓	
(OVER)			

BMB
3/18/2010


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 2nd day of April, 2010.


(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130286 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130286

MARCH 08, 2010 ✓

OPERATOR'S NAME:

SMETZOF-STANLEY

OPERATOR'S NUMBER: 5002

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

L

O.L. #: L

DEPT/AGENCY: NPLI

CASE/REPORT:

TEST TYPE: U

ALCO TARGET VALUE: .083 ✓

ALCO S/N: X172959 ✓

--- BREATH ANALYSIS ---

.083 ADJUSTED FOR 28.50 in
ALCO TARGET .079 17:27
BLANK TEST .000 17:28
INTERNAL STANDARD VERIFIED 17:28
ALCO TU 28.50 in .073 17:29
BLANK TEST .000 17:29
SUBJECT SAMPLE .000 17:30
BLANK TEST .000 17:31
ALCO TU 28.50 in .075 17:31
BLANK TEST .000 17:32

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130286 ✓

MARCH 08, 2010 ✓
TIME 17:22

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c

BAROMETER: 28.52 in

FLOW DETECTOR: OKAY

PUMP
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmnop
qrstuvwxyz{|}~@